
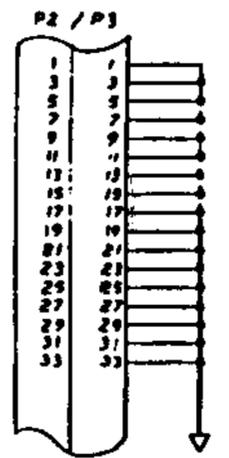
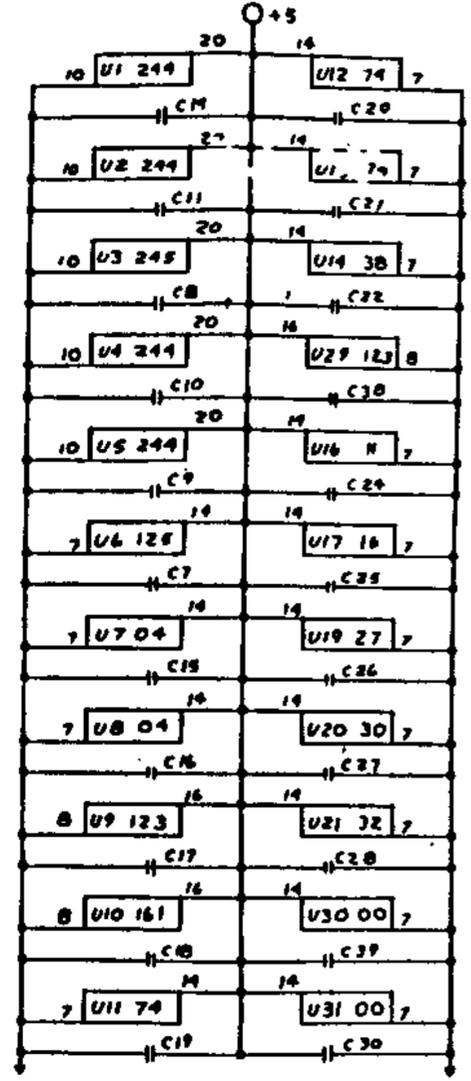


NOTE: ALL OF THE FIGURE BELOW IS 74LS SERIES TTL. ALL CAPS ARE 0.01µF.

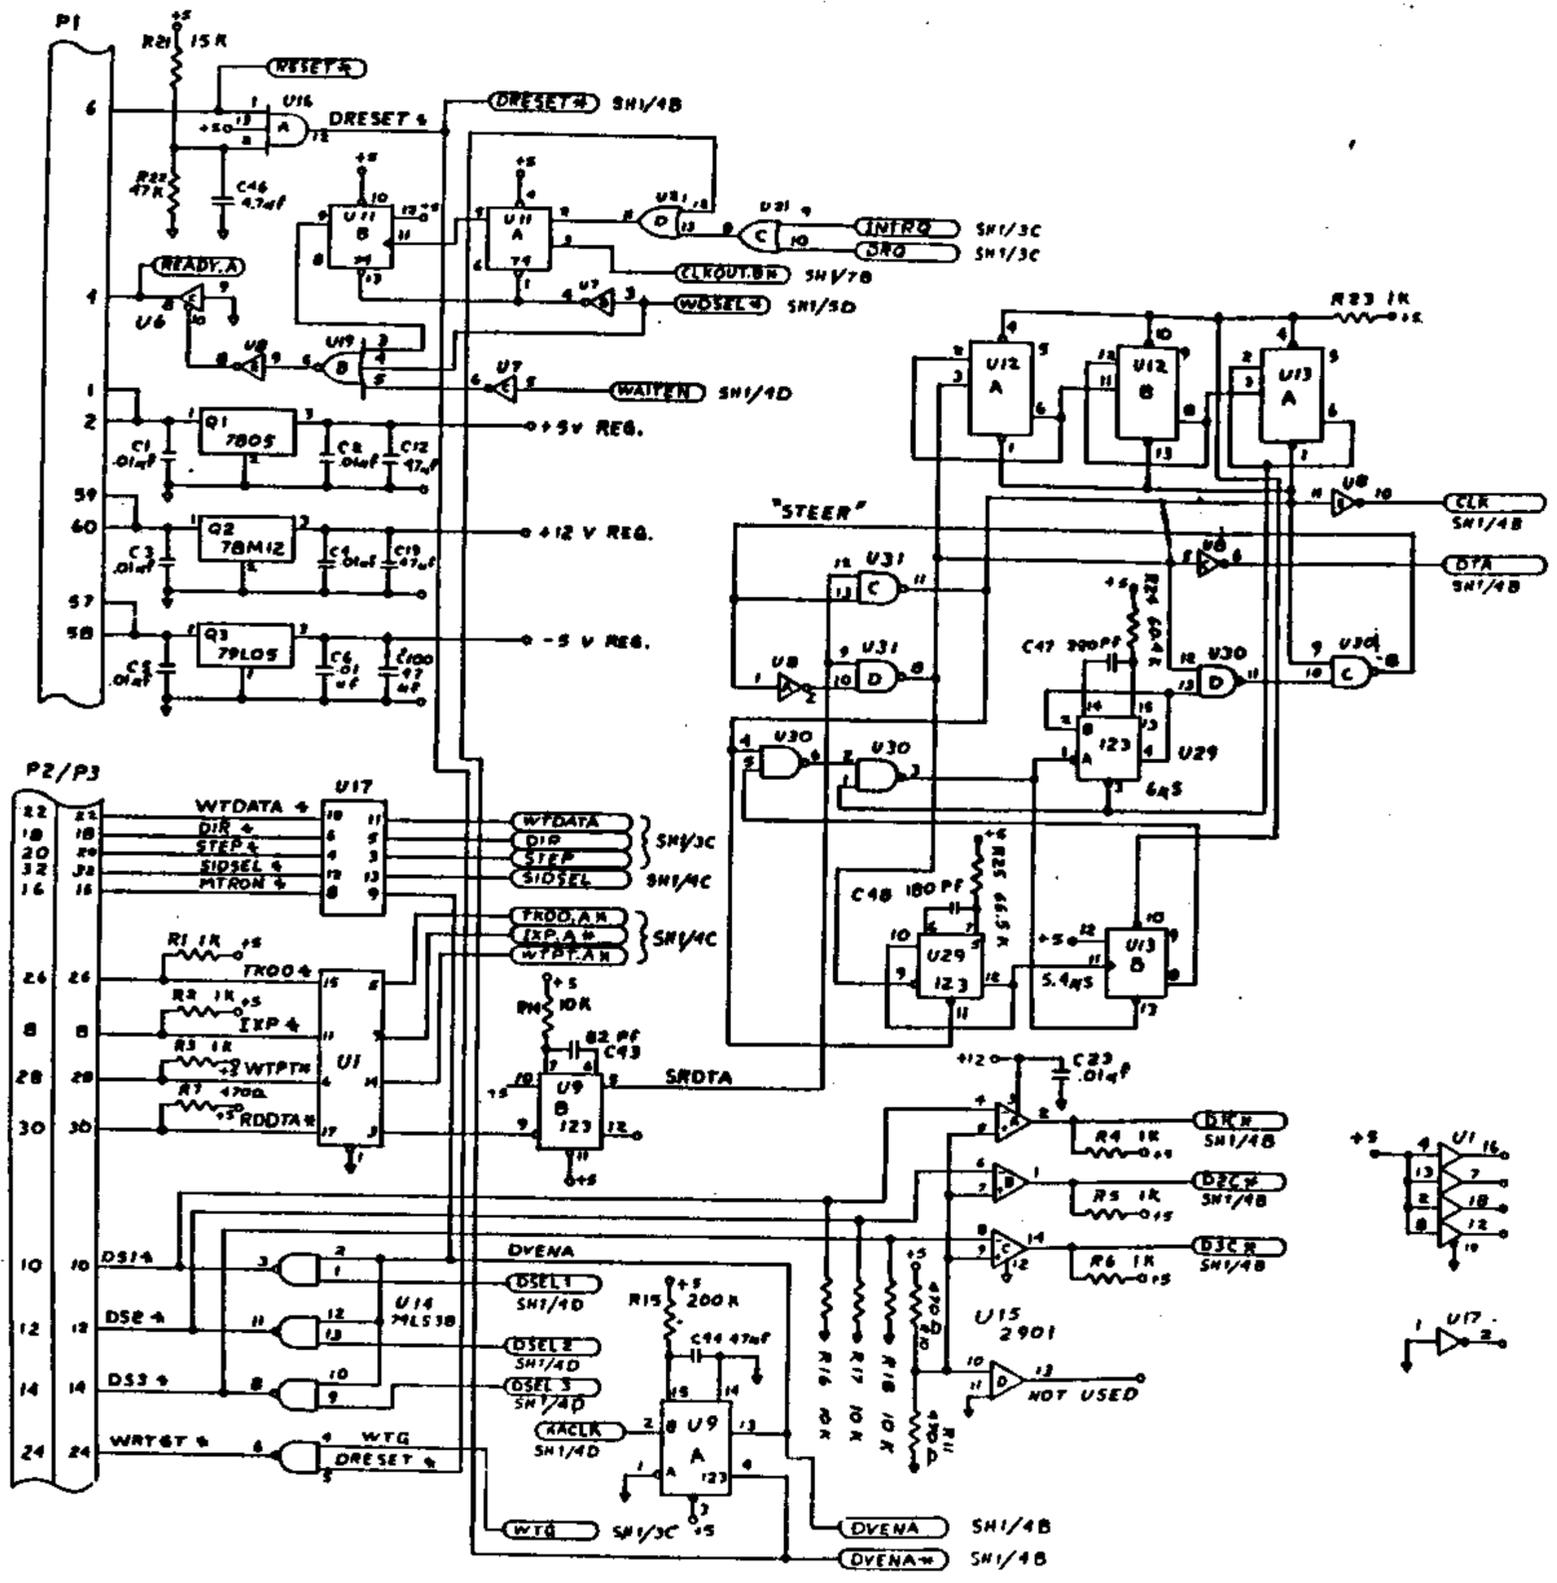

DESIGNER IDENT NUMBER	
NAME	ROOM

TEXAS INSTRUMENTS	REV. 3-15-82	1039340